

# SARS-CoV-2/FluA/FluB+ ADV/RSV Antigen Combo Rapid Test Kit (LFIA)

For self-testing



**5 in 1**  
One step process differentiate 5 infections



**Easy process**  
Easy operation, no extra equipment needed



**Rapid**  
Results in 15-20 minutes



**Easy storage**  
Room temperature storage and transportation



**Effective for mutation viruses**  
Cover different virus strain types



**Integrated strip design**  
Multiple test lines combined in one strip to facilitate the procedure

## Test Kit contents



Test Cassette



Sterile Anterior  
Nasal Swab



Lysis Buffer  
and Dropper(430µL)




Bio-Safety  
Bag



Instructions  
for Use

## Testing Procedure

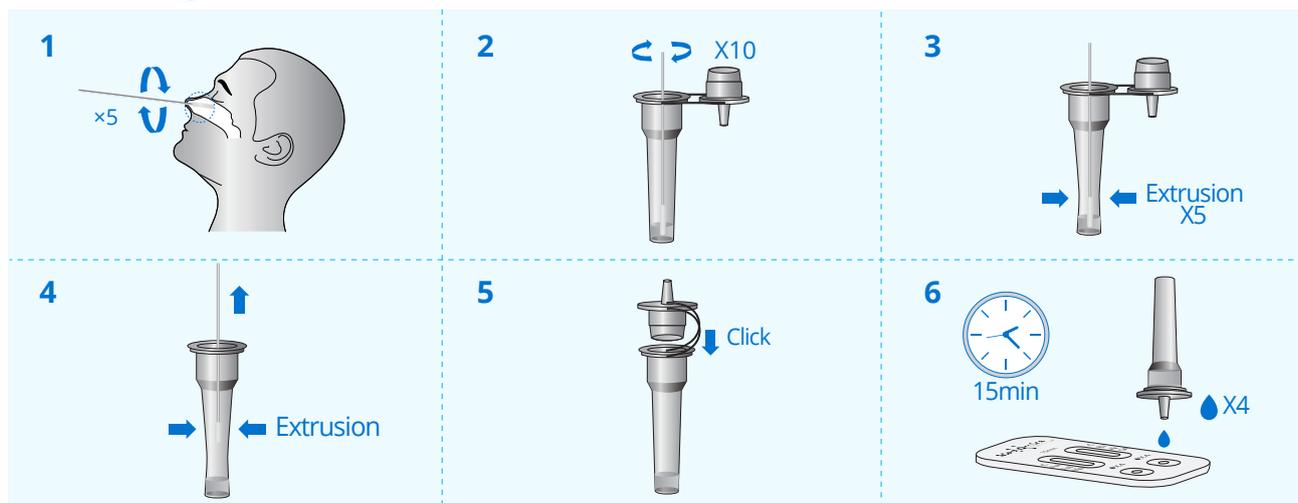

JIANGSU MEDOMICS MEDICAL TECHNOLOGY CO., LTD.  
BUILDING 01, PHASE 6, NO.71, XINGHUI ROAD, JIANGBEI NEW AREA, NANJING, 210000,  
JIANGSU, P.R. CHINA  
TEL: (+86)025-58601060/ (+86)025-58601213  
FAX: 025-58601060  
WEB: WWW.MEDOMICS-DX.NET  
E-MAIL: OVERSEAS@MEDOMICS-DX.COM / SUPPORT@MEDOMICS-DX.COM



**Storage:**  
2-30°C



**Detection Time:**  
15-20 minutes




**Shelf Life:**  
36 months

## Display of Results/Expected Values

For SARS-CoV-2&Flu A/B (Left)


“C”: Control Line “FluA”: Influenza A Test Line

“FluB”: Influenza B Test Line “nCoV”: SARS-CoV-2 Test Line “S”: Sample Well

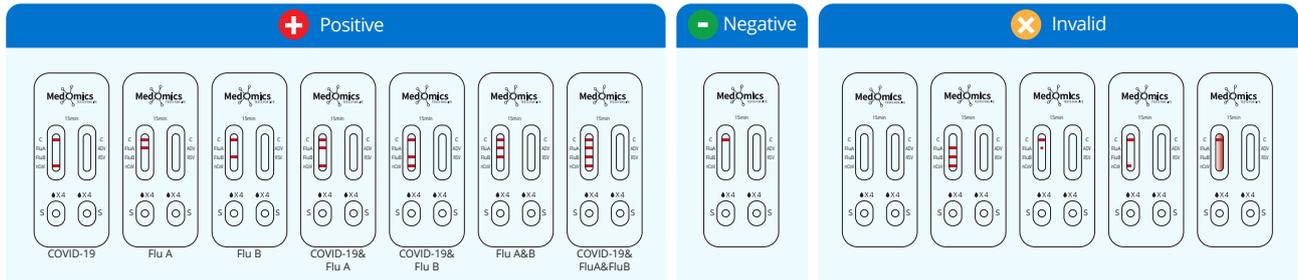

For ADV/RSV/SA (Right)

“C”: Control Line “ADV”: ADV Test Line “RSV”: RSV Test Line “S”: Sample Well

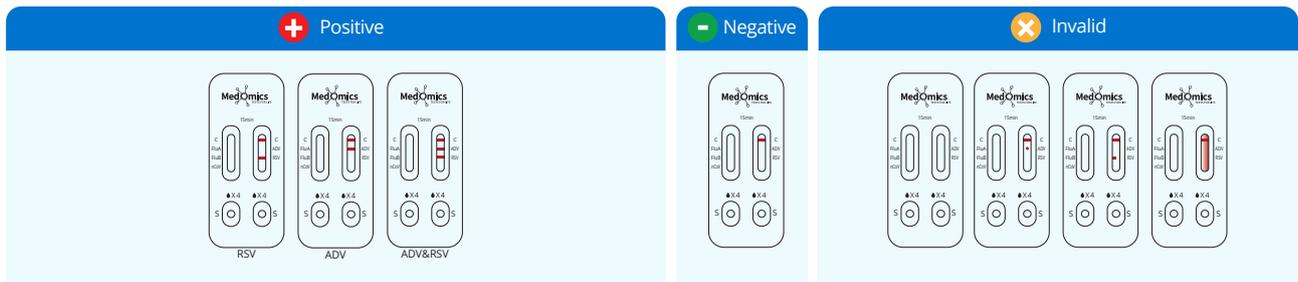

## Specifications

REF	Components Specification	Test Cassette	Sterile Anterior Nasal Swab	Lysis Buffer and Dropper(430μL)	Bio-Safety Bag	Instruction for use
123143-01-102	1 pc/Box	1	1	1	1	1
123143-02-102	2 pcs/Box	2	2	2	2	1
123143-05-102	5 pcs/Box	5	5	5	5	1
123143-20-102	20 pcs/Box	20	20	20	20	1



JIANGSU MEDOMICS MEDICAL TECHNOLOGY CO., LTD.  
BUILDING 01, PHASE 6, NO.71, XINGHUI ROAD, JIANGBEI NEW AREA, NANJING,210000,  
JIANGSU, P.R. CHINA  
TEL: (+86)025-58601060/ (+86)025-58601213  
FAX: 025-58601060  
WEB: WWW.MEDOMICS-DX.NET  
E-MAIL: OVERSEAS@MEDOMICS-DX.COM / SUPPORT@MEDOMICS-DX.COM

MK-DA-020  
Version: A/3  
Effect Date: 2025-09-10